
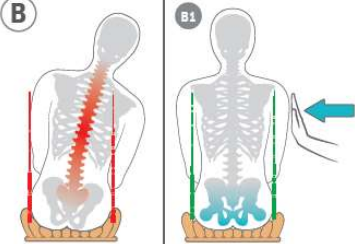




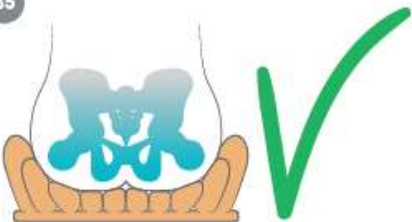


STARlock Cushion Setup Guide

	<p>Open valve above red bulb on STARlock</p>
	<p>Press the button on the bulb for 5 seconds. Sit on the cushion and press again for 5 seconds to ensure all air is removed from the locking system.</p>
	<p>Open the silver valve on the cushion corner by turning it anticlockwise</p>
	<p>Inflate STAR cushion full and leave to rest for 10 minutes with the valve open</p>
	<p>Close the silver valve by turning clockwise</p>
	<p>Position the person on the cushion and conduct a bottoming-out test to ensure there is 2-3cm of air below the Ischial Tuberosities</p>
	<p>If cushion is overinflated, turn the valve anticlockwise to release air until 2-3 cm of air remains under Ischial Tuberosities</p>
	<p>When correct height is achieved ensure silver valve is closed by turning it clockwise</p>

	<p><i>If a pressure free zone is required, use an Immedia glove to insert a foam block under desired offload area. Leave foam in glove in the desired location</i></p>
	<p>Correct posture as required and stabilise person in desired position</p>
	<p>Use the red bulb to activate the cell lock. Pump 20 times to inflate lock. This will lock all cells in position</p>
	<p>Conduct a bottoming out test to ensure 2-3cm of air under the Ischial Tuberosities</p>
	<p>When ideal positioning has been achieved, close the valve above the red bulb and place bulb in the front pocket</p>
	<p><i>If a pressure free zone was created, remove the foam block by pulling out the Immedia glove</i></p>
	<p>Cushion is set up and ready for use. Conduct regular bottoming out checks and re-set cushion as required</p>