
## STAR Cushion 'Bottoming Out' Inflation Test






- 1. Place the STAR Cushion with cover onto the chair, orientated correctly as marked on the cushion
- 2. Locate the silver valve on the left front side of the cushion
- 3. Open the valve by turning anticlockwise

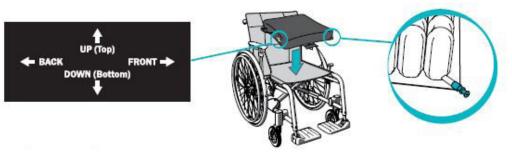


4. Attach the pump to the valve and pump to inflate the cushion to maximum



- 5. Remove the pump
- 6. Leave the valve open and let the cushion sit untouched for
- 5 minutes to allow the air to equalise
- 7. Close the valve by turning clockwise




8. Position the Client on the cushion positioned as desired



Novis Healthcare Pty Ltd Unit 12/12 Mars Road Lane Cove NSW 2066 Australia

- 9. Perform a bottoming out/inflation test
  Apply the MaxiGlide Glove to your hand
  - Insert your hand facing down between the Client and the cushion
  - Locate your fingers under the ischial tuberosity
  - Move your fingers up and down to determine height of the cushion
  - Desired height is 2-3cm of inflation under the ischial tuberosities



- □ If less than 2cm inflation open the valve and use the pump to add more air into the cushion
- □ If greater than 3cm open valve and release some air from the cushion
- Complete the bottoming out test again until desired height of 2-3cm under the Ischial Tuberosities is reached
- Remove hand and glove



10. Recheck cushion using bottoming out test at regular intervals to ensure appropriate inflation is maintained



E orders@novis.com.au W novis.com.au

Inflation is r

ABN 45 102 735 491

NDIS 4050019411